


PATIENT

Last Name/Patient ID _____

First Name _____

DOB / / Male Female

Weight _____ Height _____

Dx _____

Right Left Bilateral

COMPANY

Name _____

Contact Name _____

Phone _____ Fax _____

E-mail _____

BILLING / SHIPPING

BILLING

Address _____

City _____

ST/Prov _____ Zip _____

Shipping address same as billing? Yes No

SHIPPING

Address _____

City _____

ST/Prov _____ Zip _____

PO # _____

Order confirmation: Fax E-mail

FedEx SHIPPING OPTIONS
Need by Date

Ground®FREE

2 Day® A.M. 10:30 a.m. or noon 2nd business day\$30.00

Priority Overnight® 10:30 a.m. next business day\$55.00

First Overnight® 8:00 a.m. next business day\$100.00

Next Day \$75.00

Same Day \$100.00

24 Rush Fab Shipping charges apply separately

CASTS

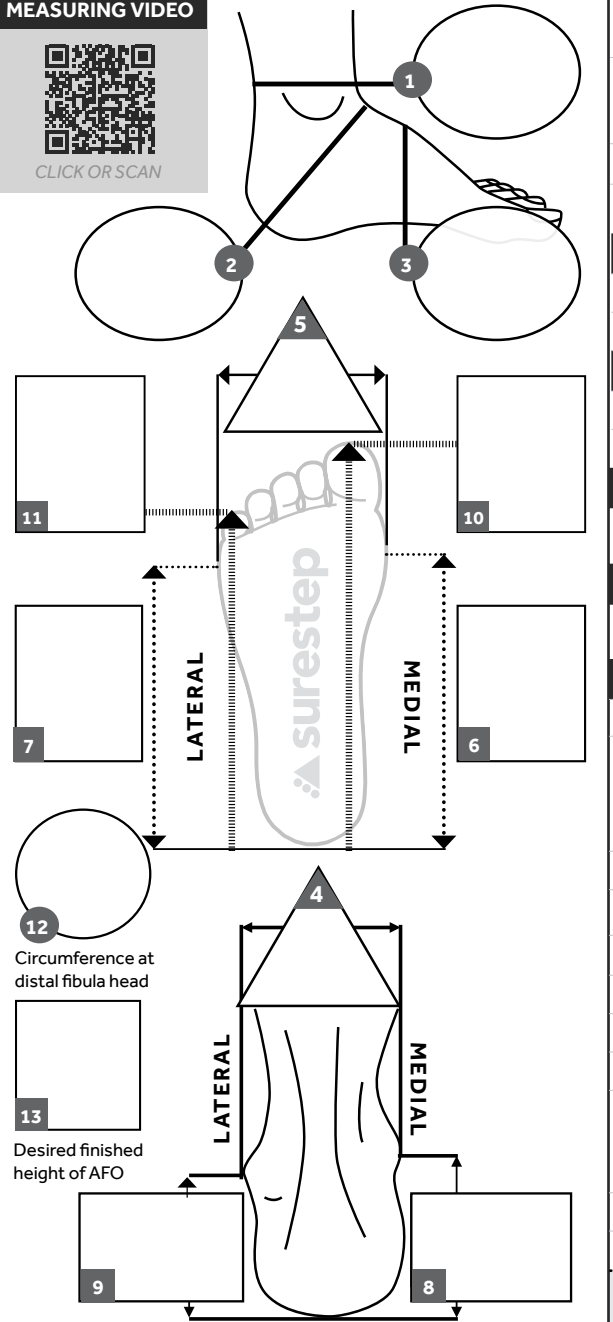
Sending Casts: Yes No

Return impressions pre-modifications \$20.00/pr.

Send casts: 17530 Dugdale Dr. South Bend, IN 46635

MEASUREMENTS

● Circumference ▲ Width ■ Distance

MEASURING VIDEO


* If number 5 measurement is 3" or greater, a cast is required.

DEVICE STYLE

UCBL

SMO

Floor Reaction AFO

Solid Ankle AFO

Posterior Leaf AFO

Hinged AFO, Custom Fabricated

HINGE

Surestep Free Motion Surestep DA

Tamarack Free Motion Tamarack DA

Gaffney

Other: _____

STOPS

Surestop Snapstop Elite Plastic

Other: _____

CORRECTION

Cast Modifications Neutral/90 As casted

Heel: _____ Ankle: _____ Forefoot: _____

PLASTIC OPTION

Polypropylene Polyethylene Copolymer Other: _____

Thickness: _____ Color: _____

PATTERN CHAFE (D-RINGS)

Plastic Standard Dacron Optional, no charge

STRAP COLOR DORSAL PAD

Dorsal Pad Standard Neoprene Pad Optional, no charge

ADDITIONS/MODIFICATIONS (Additional charges may apply, see price list)

Liner

Volara (white) Puff

Other: _____

1/8" 3/16" 1/4"

Dorsum Wing

Medial Lateral

Heel Post

Rigid Plastic Crepe

Carbon Fiber Reinforcement

T-Strap

Medial Lateral

Duraflex Polyethylene

Condyle Extension

Medial Lateral

Molded Inner Boot

MPE Duraflex Foam

1/16" 3/32" 1/8"

TRIMLINE

Height: SMO Full

Boot: Short Surestep Full Length Footplate

Pre-Tibial Shell

Internal (tuck-in)

MPE Duraflex

3/32" 1/8"

External (overlap)

Material same as device

Specify thickness: _____

Walking Base (Attached to AFO)

Open Heel

NOTES